


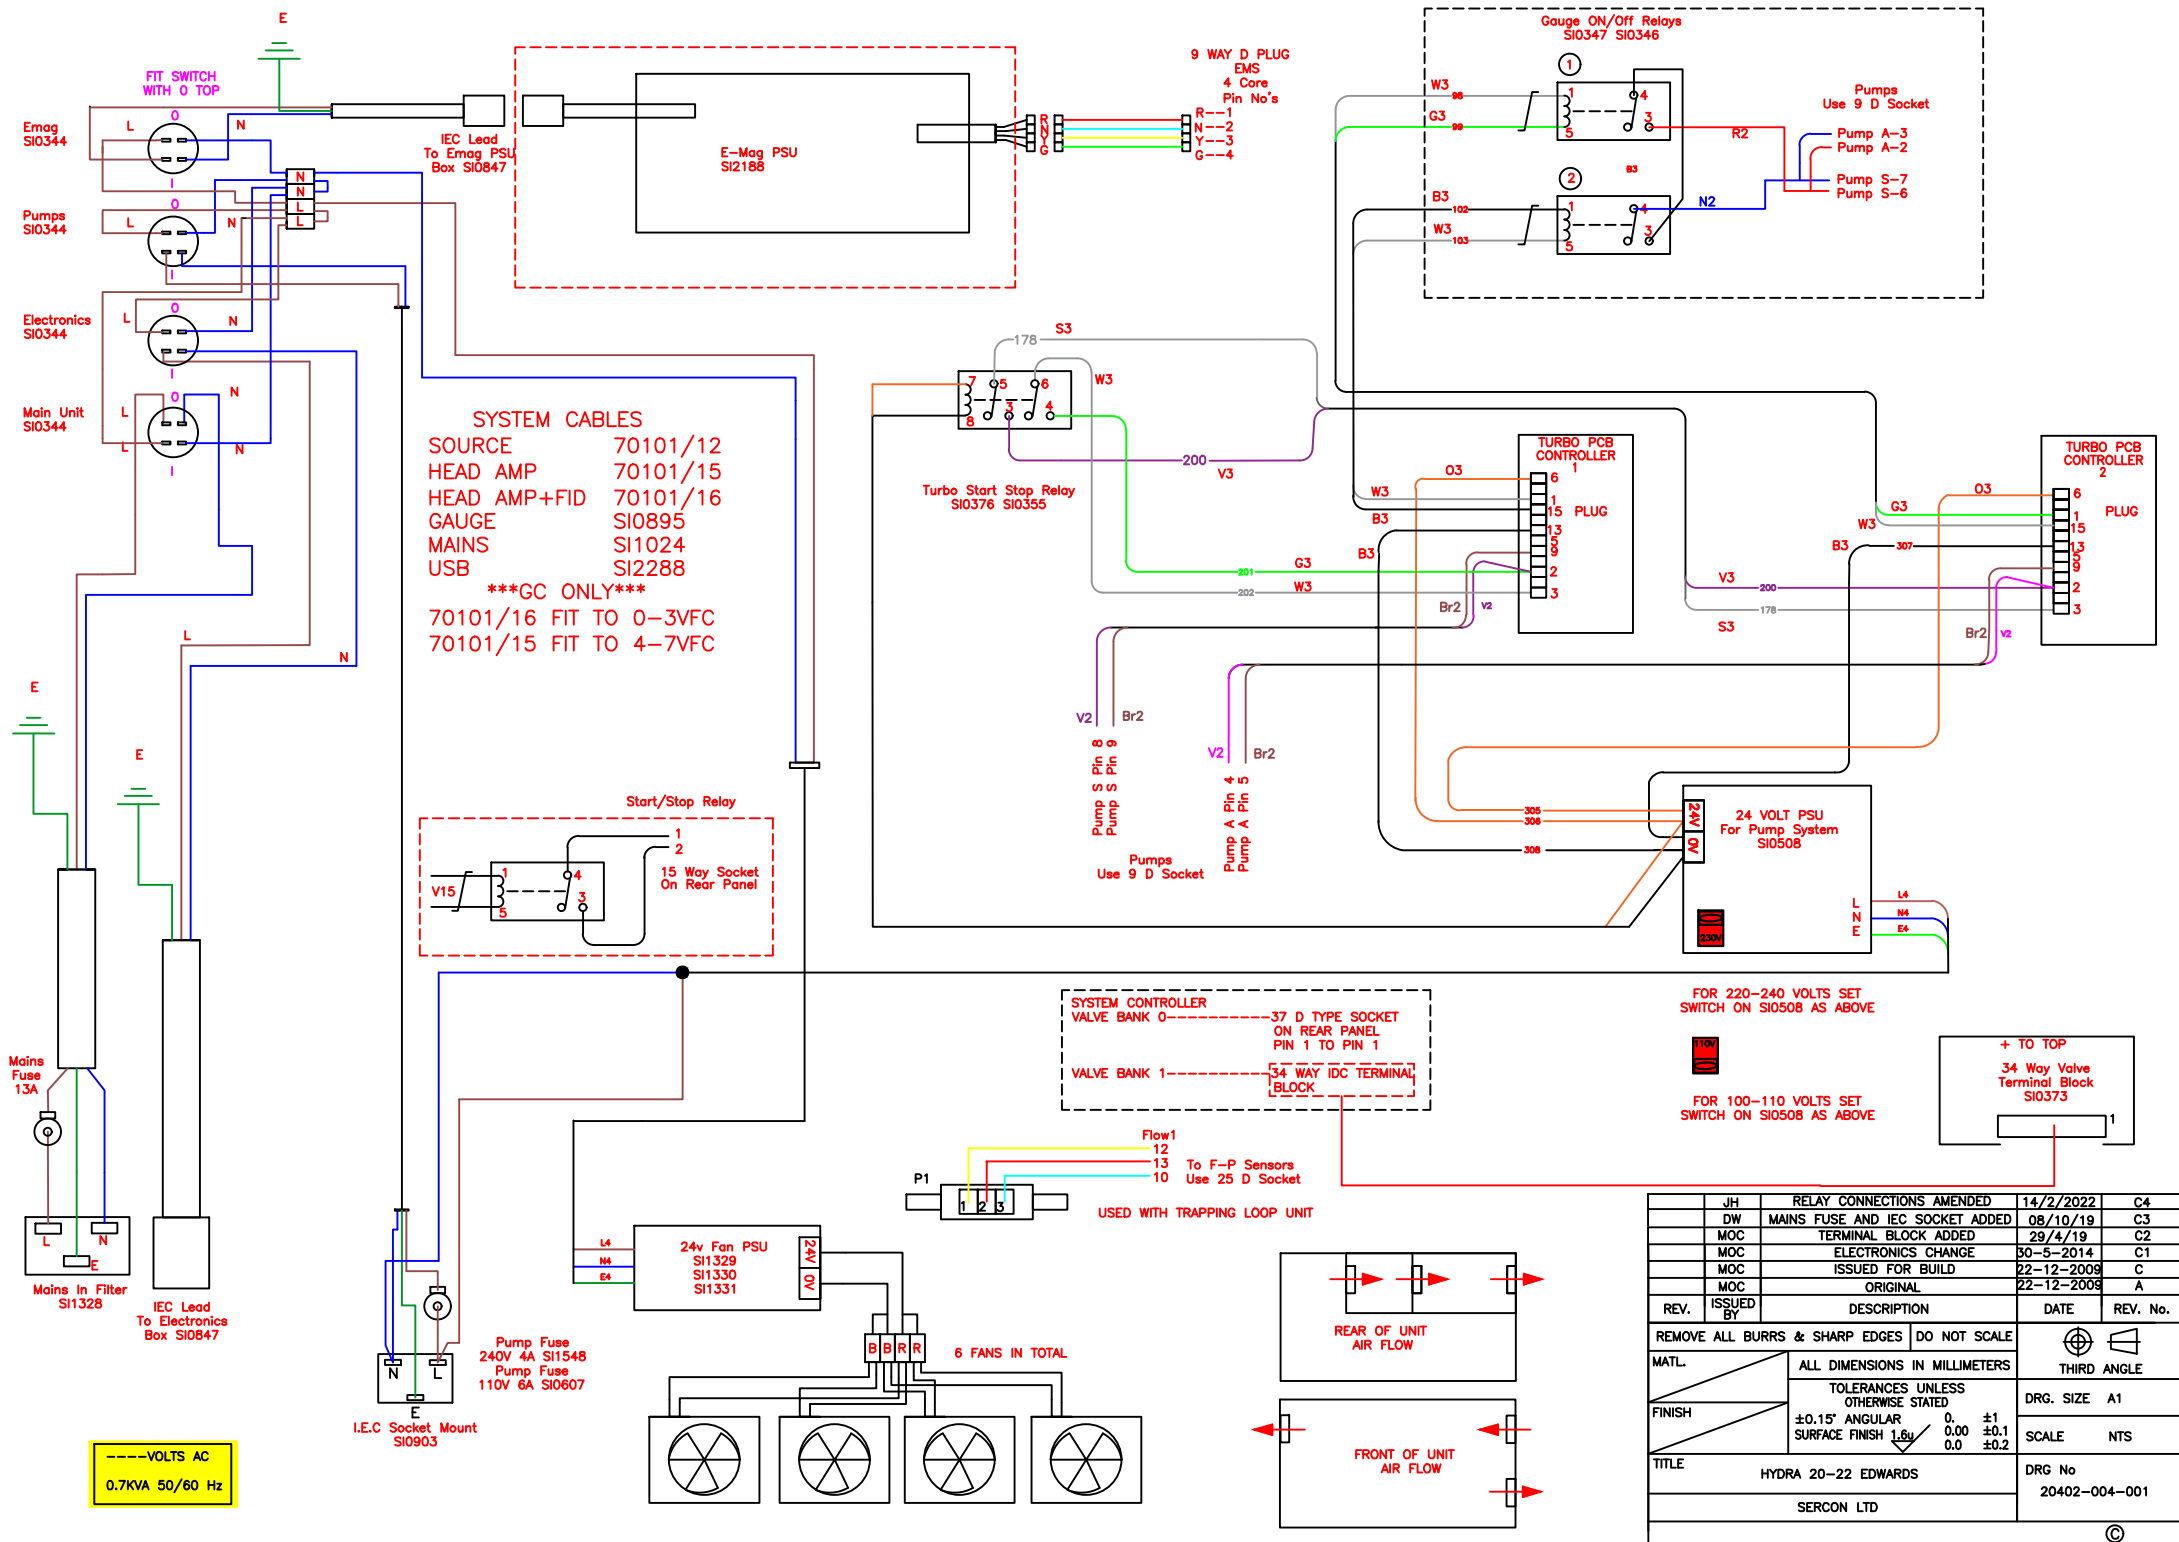

-----VOLTS AC
0.7KVA 50/60 Hz

JH	RELAY CONNECTIONS AMENDED	14/2/2022	C4
DW	MAINS FUSE AND IEC SOCKET ADDED	08/10/19	C3
MOC	TERMINAL BLOCK ADDED	29/4/19	C2
MOC	ELECTRONICS CHANGE	30-5-2014	C1
MOC	ISSUED FOR BUILD	22-12-2009	C
MOC	ORIGINAL	22-12-2009	A
REV.	DESCRIPTION	DATE	REV. No.
1	REMOVE ALL BURRS & SHARP EDGES	DO NOT SCALE	
MATL	ALL DIMENSIONS IN MILLIMETERS		
FINISH	TOLERANCES UNLESS OTHERWISE STATED	DRG. SIZE	A1
	±0.15° ANGULAR	0.00 ±0.1	SCALE
	SURFACE FINISH 1.6	0.0 ±0.2	NTS
TITLE	HYDRA 20-22 EDWARDS	DRG No	20402-004-001
	SERCON LTD		
			©